

AD-A070 704

NAVAL WEAPONS CENTER CHINA LAKE CA
WAVELENGTH REPEATABILITY OF A CARY MODEL 14R SPECTROPHOTOMETER.(U)
MAY 79 M E HILLS
NWC-TP-6109

F/G 20/6


UNCLASSIFIED

NL

| OF |
AD
A070 704



END
DATE
FILMED
8-79
DDC

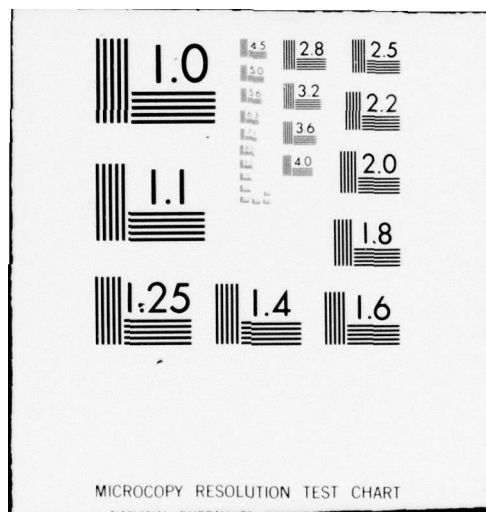

ADA070704

LEVEL

14
NWC-TR-6109

a/z

6
**WAVELENGTH REPEATABILITY
OF A CARY MODEL 14R
SPECTROPHOTOMETER.**

9 Research Rept.

10 by
Marian E. Hills
Research Department

11 MAY 1979

12 20p.

DDC
RECEIVED
JUL 2 1979
C
JFC

**NAVAL WEAPONS CENTER
CHINA LAKE, CALIFORNIA 93555**



Approved for public release;
distribution unlimited.

403019

JB

79-06-29 016

DDC FILE COPY

Naval Weapons Center

AN ACTIVITY OF THE NAVAL MATERIAL COMMAND

FOREWORD

This report describes a study made to determine the precision of wavelength measurements made with a Cary Model 14R spectrophotometer.

This report was reviewed for technical accuracy by Allen L. Olsen and H. E. Bennett.

Approved by
E. B. ROYCE, *Head*
Research Department
31 May 1979

Under authority of
W. L. HARRIS
RAdm., U. S. Navy
Commander

Released for publication by
R. M. HILLYER
Technical Director

NWC Technical Publication 6109

Published by Technical Information Department
Collation Cover, 8 leaves
First printing 160 unnumbered copies

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER NWC TP 6109	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) WAVELENGTH REPEATABILITY OF A CARY MODEL 14R SPECTROPHOTOMETER		5. TYPE OF REPORT & PERIOD COVERED Research Report
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) Marian E. Hills		8. CONTRACT OR GRANT NUMBER(s)
9. PERFORMING ORGANIZATION NAME AND ADDRESS Naval Weapons Center China Lake, CA 93555		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS
11. CONTROLLING OFFICE NAME AND ADDRESS Naval Weapons Center China Lake, CA 93555		12. REPORT DATE May 1979
		13. NUMBER OF PAGES 14
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) UNCLASSIFIED
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Approved for public release; distribution unlimited.		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Spectrophotometer Wavelength Precision		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) See back of form.		

DD FORM 1 JAN 73 1473

EDITION OF 1 NOV 65 IS OBSOLETE
S/N 0102-LF 014-6601

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

79 06 29 016

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)

(U) *Wavelength Repeatability of a Cary Model 14R Spectrophotometer*, by Marian E. Hills. China Lake, Calif., Naval Weapons Center, May 1979. 14 pp. (NWC TP 6109, publication UNCLASSIFIED.)

(U) In our laboratory Cary spectrophotometers are used to measure the transmittance of optical components and materials. One instrument in particular, a Cary Model 14R spectrophotometer, is used to calibrate narrow-band interference filters. The precision of the wavelength measurements was determined using the D_β line of the deuterium source lamp as a wavelength standard.

D SUB BETA

Accession For	
NTIS	GRA&I
DDC	TAB
Unannounced	
Justification	
By	
Distribution/	
Availability Codes	
Dist	Avail and/or special
A	

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)

INTRODUCTION

In our laboratory Cary spectrophotometers are used to measure the transmittance of optical components and materials. One instrument in particular, a Cary Model 14R spectrophotometer, is used to calibrate narrow-band interference filters used in a rocketborne ozonesonde. Preliminary assessment of repetitive scans of a filter showed that the center of the bandpass appeared to shift to longer wavelengths in an orderly manner. This raised the question of whether the instrument was shifting its calibration (due perhaps to temperature changes), whether some temperature effect was shifting the bandpass of the interference filter, or whether some other effects or combination of effects was occurring.

This report deals with studies made to determine the precision of wavelength measurements made with the spectrophotometer and to show how the instrument might be shifting its calibration during operation.

EXPERIMENTAL

The 4860 Å line (D_{β}) of the deuterium source lamp was used as the wavelength standard. It was found that the lamp contained hydrogen as well as deuterium (Figure 1). Temperatures were measured with Type K thermocouples; the thermocouples were not calibrated because the change in temperature with time and instrument usage -- not temperature per se -- was sought.

The wavelength temperature coefficient of the spectrophotometer is stated to be 0.3 Å per degree Celsius.¹ However, no information is given about where the temperature changes should be measured if the entire monochromator is not at the same temperature. Since knowledge about specific locations at which thermocouples should be placed was not available, the decision was made not to open the monochromator

¹ Varian Company. *Instructions for Cary Recording Spectrophotometer Model 14R*, Varian, Instrument Division, Palo Alto, Calif., Handbook (undated), p. 2.

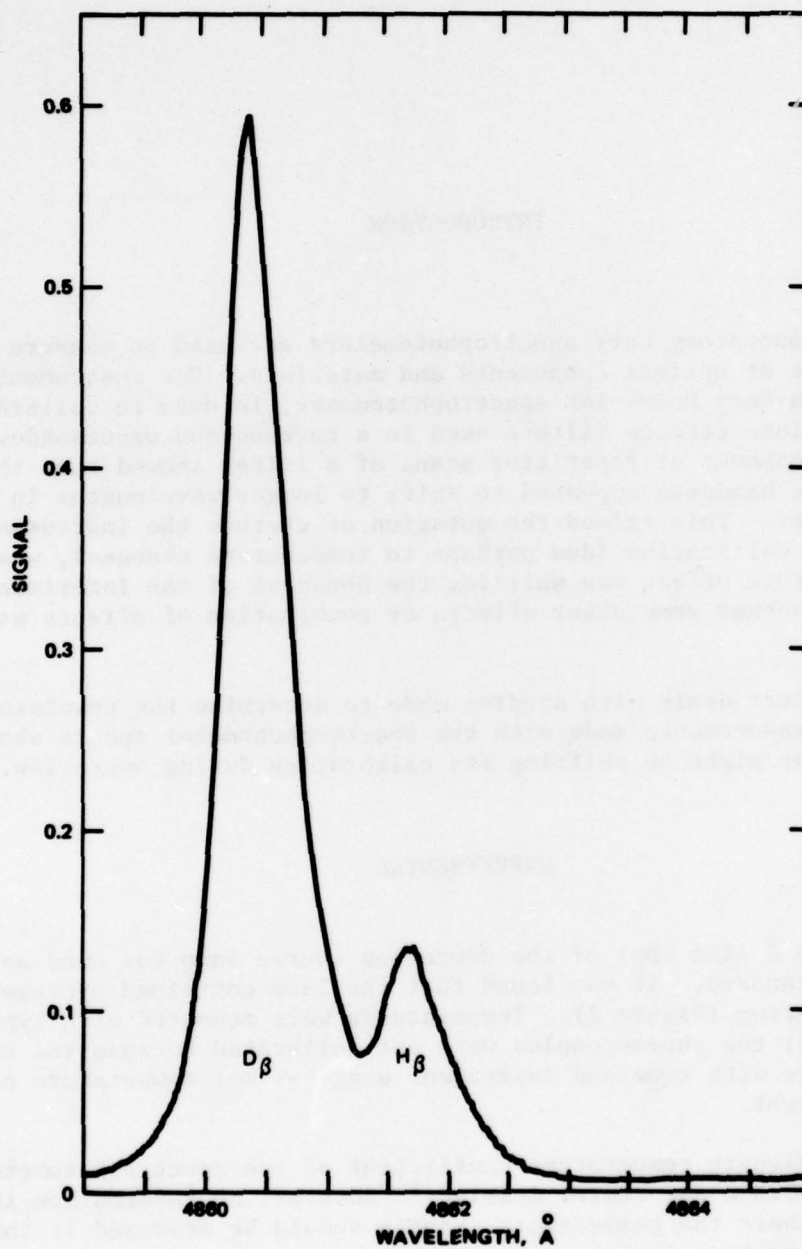


FIGURE 1. D β and H β Spectral Lines of Source Lamp.

housing and expose the elements to dust in order to place thermocouples inside of the monochromator housing, but rather to place thermocouples on the exterior of the housing. Thermocouples were placed on the lower left front wall of the housing and on the top of the housing at the right rear (under the heat shield); thermocouples were also placed in the sample compartment. One thermocouple was hung in air in the vicinity of the spectrophotometer.

The output from the thermocouples was read with a data logger which recorded the temperatures directly with a resolution of 0.1°C .

Two scanning speeds were employed: $1/4 \text{ \AA/sec}$ and $1/8 \text{ \AA/sec}$; the chart was driven at 5 in./min. The standard chart paper for the instrument has three divisions per inch on the wavelength axis. Thus the combinations of scanning speeds with chart speed resulted in the analog record having 1 \AA/barleycorn or $1/2 \text{ \AA/barleycorn}$ (a barleycorn is $1/3$ -inch). Since no readily available scales divide one-third of an inch into 5 or 10 parts, scales having 15 divisions/in. and 30 divisions/in. were made with a Gerber plotter. These scales are reproduced in Figure 2 for the convenience of others.

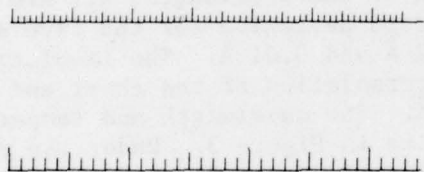


FIGURE 2. Scales of 30 Divisions Per Inch and 15 Divisions Per Inch.

In order to take the backlash out of the wavelength drive mechanism, the following regime was employed (the particular spectrophotometer used has a two-speed motor which gives one-half or one-fourth of the speed of the motor usually supplied with the instrument):

- a. Scan from 5400 \AA to 4900 \AA at 50 \AA/sec or 25 \AA/sec .
- b. Scan from 4900 \AA to $\sim 4875 \text{ \AA}$ at $2 \frac{1}{2} \text{ \AA/sec}$ or $1 \frac{1}{4} \text{ \AA/sec}$.
- c. Scan from $\sim 4875 \text{ \AA}$ to 4859 \AA at $1/4 \text{ \AA/sec}$ or $1/8 \text{ \AA/sec}$.
- d. Record analog data from 4865 \AA to 4859 \AA .

The instrument was equipped with a transmittance slidewire and operated in the reference mode. The reference beam was blocked with paper and tape; the reference compartment was kept closed as was the sample compartment. A piece of black tape was placed across the lower portion of the wavelength counter window in order to reduce the parallax error.

The wavelengths at which the line attained one-half of its peak value were read from the 4859 Å position marked on the chart. The line position, designated by λ_c , was then calculated (the average of the wavelengths at the two half-power points).

RESULTS AND DISCUSSION

After the spectrophotometer had been warmed up for one hour and a few preliminary scans had been made, scans were made at approximately 15-minute intervals for the next hour and at 30-minute intervals for the next 6 1/2 hours, at which time four scans were made in rapid succession. Table 1 gives the band position for the D_β line and the temperature recorded from the thermocouple attached to the front wall of the monochromator housing. For the twenty-two scans tabulated the mean and standard deviation of the wavelength, λ_c , are 4860.53 Å and 0.19 Å. The mean and standard deviation for the five scans numbered 18A through 22A are 4860.32 Å and 0.01 Å. The tabulation of wavelength to 0.01 Å resulted from interpolation of the chart and is not meant to imply an accuracy of 0.01 Å. The wavelength and temperature data are plotted as a function of time in Figure 3. Under the conditions at which the data shown in Figure 3 were collected the values of λ_c tend to decrease as the temperature of the front wall of the monochromator increases unless scans are repeated in rapid succession.

Another set of scans was made over a period of two days to confirm the previous results and to search for conditions under which scans made in quick succession would give the same position for the D_β line and not an increasing value. The data from the first day are tabulated in Table 2; they are plotted in Figure 4 except for scans made at 1/4 Å/sec. The first scan was made 16 minutes after the instrument was turned on. The mean value and standard deviation for the eighteen 1/8 Å/sec scans are 4860.59 Å and 0.16 Å. The data show the same general trends as did the earlier data.

The instrument was left on overnight. On the second day the instrument was kept scanning in wavelength (usually between ~5400 Å and ~4900 Å) during the time that scans were not being made until mid-afternoon. The data are tabulated in Table 3 and plotted in Figure 5. The temperature of the monochromator housing increased but seemed to level off near 34°C with continuous scanning. However, long before the temperature leveled

TABLE 1. D_{β} Line of Source and Temperature of Monochromator Housing.
Scanning speed: $1/8$ Å/sec.

Scan no.	Time, ^a t, min.	Wavelength, λ_c , Å	Temperature ^b °C
6A	59.95	4860.86	24.9
7A	75.27	4860.85	25.4
8A	89.97	4860.86	26.0
9A	106.25	4860.82	26.6
10A	120.05	4860.71	27.0
11A	150.05	4860.59	27.9
12A	182.82	4860.56	28.6
13A	210.23	4860.52	29.2
14A	239.90	4860.42	29.6
15A	244.47	4860.52	29.7
16A	270.00	4860.48	30.2
17A	299.87	4860.40	30.6
18A	330.08	4860.32	30.9
19A	359.93	4860.32	31.2
20A	390.07	4860.34	31.3
21A	420.60	4860.30	31.5
22A	450.22	4860.32	31.6
23A	480.72	4860.40	31.6
24A	509.87	4860.40	31.6
25A	513.13	4860.45	31.5
26A	515.93	4860.57	31.6
27A	518.80	4860.66	31.5

^a Instrument turned on at $t = 0$.

^b Measured on front wall of monochromator housing.

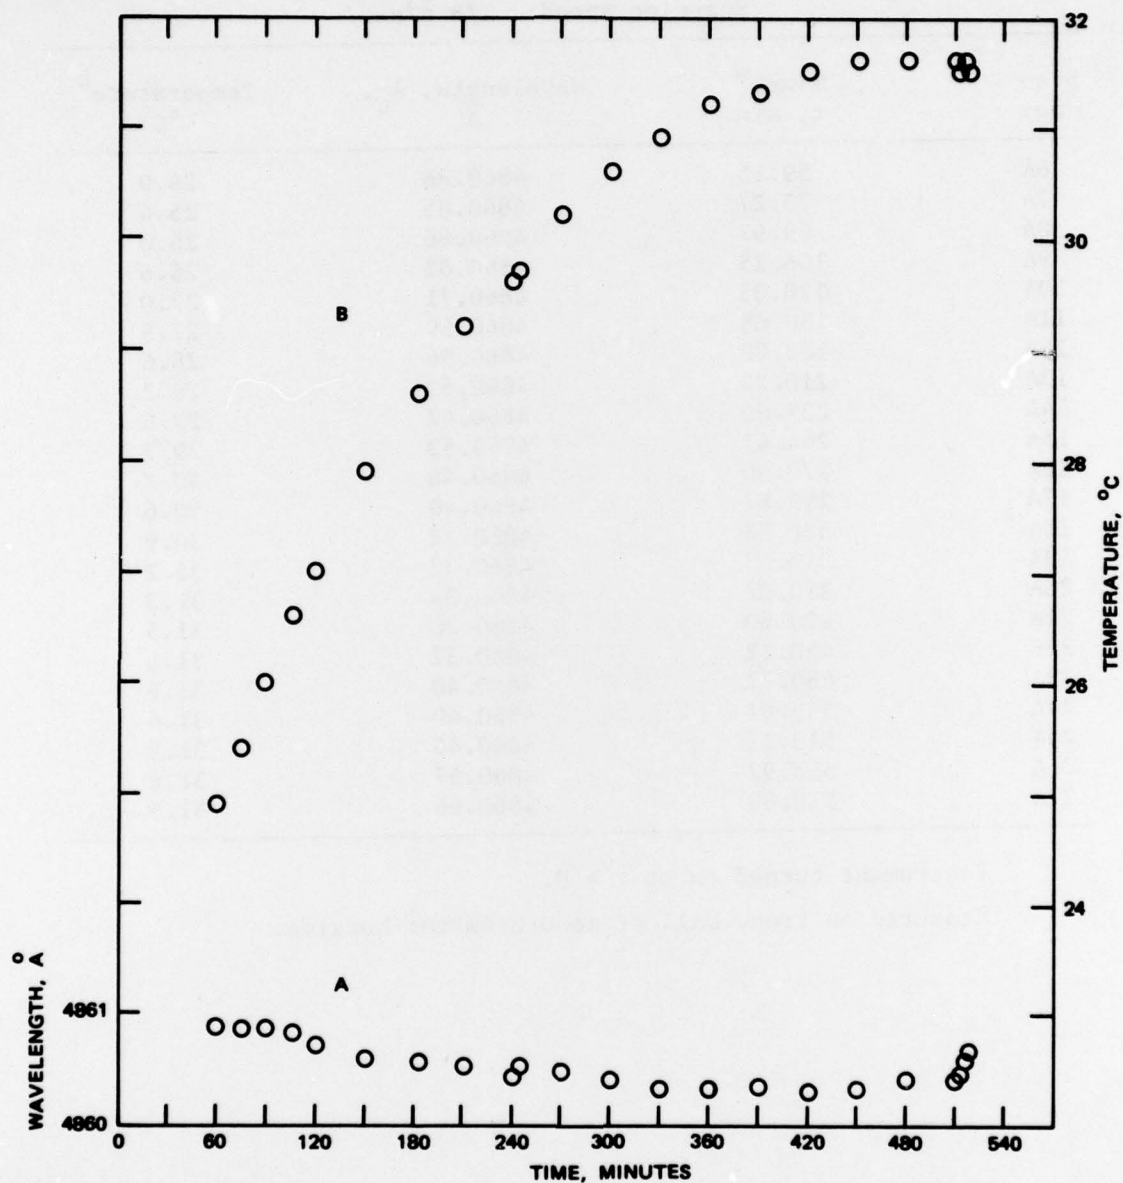


FIGURE 3. Plot of Data Tabulated in Table 1. A. Position of D_β line; B. Temperature at front wall of monochromator housing.

TABLE 2. D_{β} Line of Source and Temperature of Monochromator Housing.

Scan no.	Scan speed, Å/sec	Time, ^a t, min.	Wavelength, λ_c , Å	Temperature, ^b °C
1B	1/8	31.07	4860.70	23.7
2B	1/8	45.55	4860.77	24.1
3B	1/8	59.93	4860.80	24.6
4B	1/4	62.55	4860.79	24.7
5B	1/8	89.63	4860.64	25.7
6B	1/4	92.02	4860.67	25.8
7B	1/4	94.38	4860.78	25.9
8B	1/8	119.62	4860.80	26.8
9B	1/4	122.05	4860.79	26.8
10B	1/8	149.40	4860.75	27.6
11B	1/4	152.05	4860.70	27.7
12B	1/8	180.05	4860.62	28.3
13B	1/4	182.52	4860.57	28.3
14B	1/4	184.68	4860.70	28.4
15B	1/8	209.70	4860.58	29.0
16B	1/4	212.27	4860.62	29.1
17B	1/8	239.78	4860.48	29.5
18B	1/4	242.33	4860.58	29.5
19B	1/8	300.00	4860.40	30.0
20B	1/4	302.40	4860.50	30.1
21B	1/8	360.15	4860.35	30.5
22B	1/8	364.18	4860.40	30.5
23B	1/8	367.82	4860.52	30.5
24B	1/8	371.57	4860.59	30.6
25B	1/8	375.07	4860.68	30.7
26B	1/8	378.15	4860.74	30.8
27B	1/8	419.43	4860.48	31.0
28B	1/8	464.85	4860.35	31.0

^a Instrument turned on at t = 15 min.^b Measured on front wall of monochromator housing.

TABLE 3. D_{β} Line of Source and Temperature of Monochromator Housing.
Scanning speed: $1/8 \text{ \AA/sec}$.

Scan no.	Time, ^a t, min.	Wavelength, λ_c , \AA	Temperature, ^b $^{\circ}\text{C}$
29B	47.88	4860.40	30.3
30B	51.88	4860.44	30.3
31B	55.18	4860.54	30.4
32B	59.48	4860.62	30.4
33B	63.03	4860.77	30.5
34B	66.48	4860.88	30.6
Instrument Scanning at $1/8 \text{ \AA/sec}$ Between 34B and 35B			
35B	120.08	4861.45	32.1
36B	123.83	4861.42	32.3
37B	127.32	4861.47	32.3
38B	130.75	4861.44	32.4
39B	134.27	4861.40	32.5
40B	137.78	4861.44	32.5
41B	141.37	4861.44	32.7
42B	144.78	4861.42	32.7
43B	148.30	4861.36	32.7
44B	151.80	4861.40	32.8
Instrument Scanning at $1/8 \text{ \AA/sec}$ Between 44B and 45B			
45B	213.57	4861.43	33.4
Instrument Scanning at $1/8 \text{ \AA/sec}$ Between 45B and 46B			
46B	300.98	4861.42	33.9
47B	304.52	4861.38	34.0
48B	307.90	4861.44	34.0
49B	311.43	4861.38	34.0
50B	314.70	4861.38	33.9
Instrument Scanning at $1/8 \text{ \AA/sec}$ Between 50B and 51B			
51B	358.83	4861.38	34.1
52B	362.23	4861.41	34.1
53B	365.65	4861.34	34.1
54B	369.07	4861.35	34.1
55B	372.52	4861.37	34.2

TABLE 3. (Contd.)

Scan no.	Time, ^a t, min.	Wavelength, λ_c , Å	Temperature, ^b °C
Instrument Not Scanning Between 55B and 56B			
56B	418.97	4860.41	33.1
57B	422.40	4860.42	33.0
58B	425.70	4860.50	33.0
59B	429.13	4860.62	32.9
60B	432.47	4860.65	33.0
Instrument Not Scanning Between 60B and 61B			
61B	453.15	4860.50	32.9
62B	456.58	4860.56	32.9
Instrument Not Scanning Between 62B and 63B			
63B	526.32	4860.22	31.8
64B	529.72	4860.30	31.8

^a Instrument turned on 23.75 hr. before $t = 0$.

^b Measured on front wall of monochromator housing.

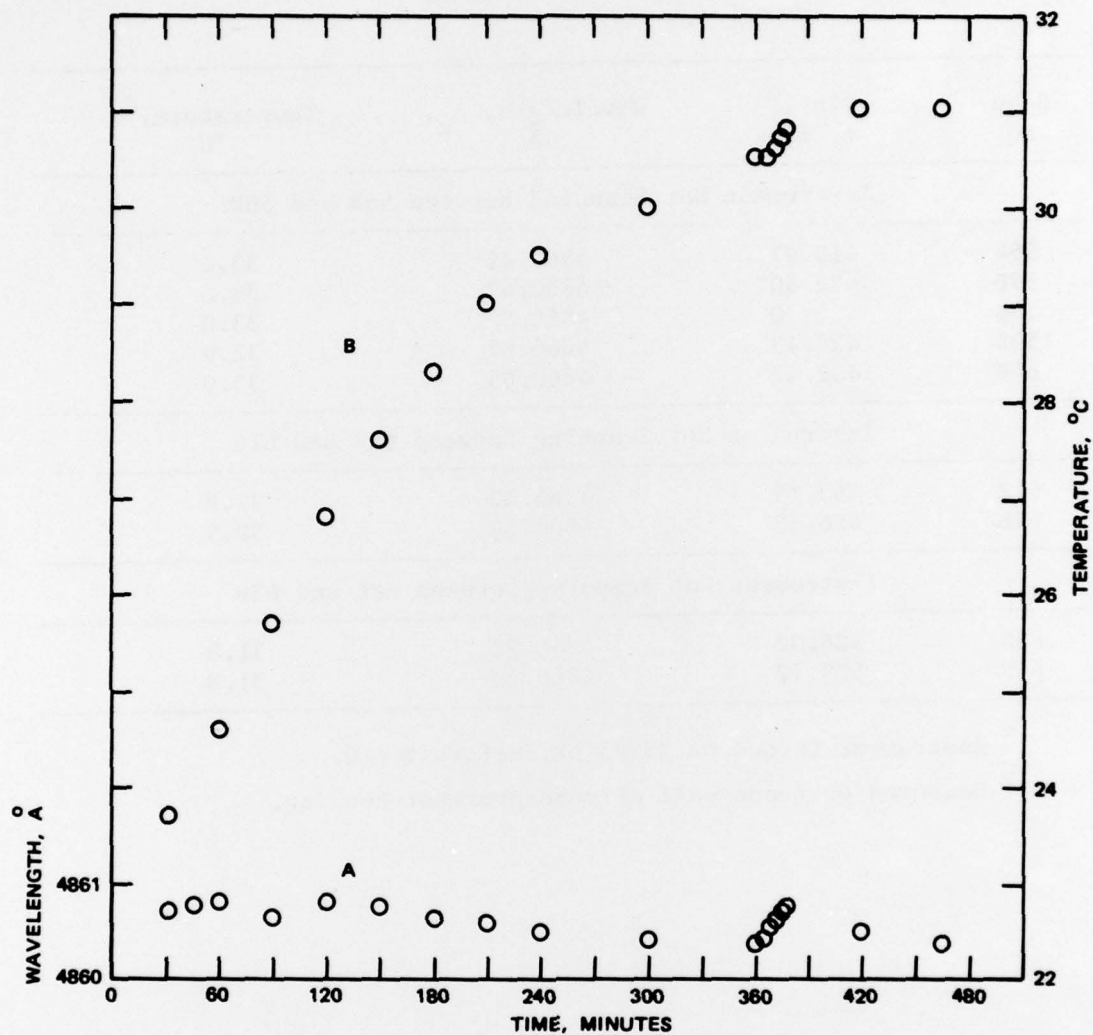


FIGURE 4. Plot of Some of the Data Tabulated in Table 2.
A. Position of D_{β} line; B. Temperature at front wall of monochromator housing.

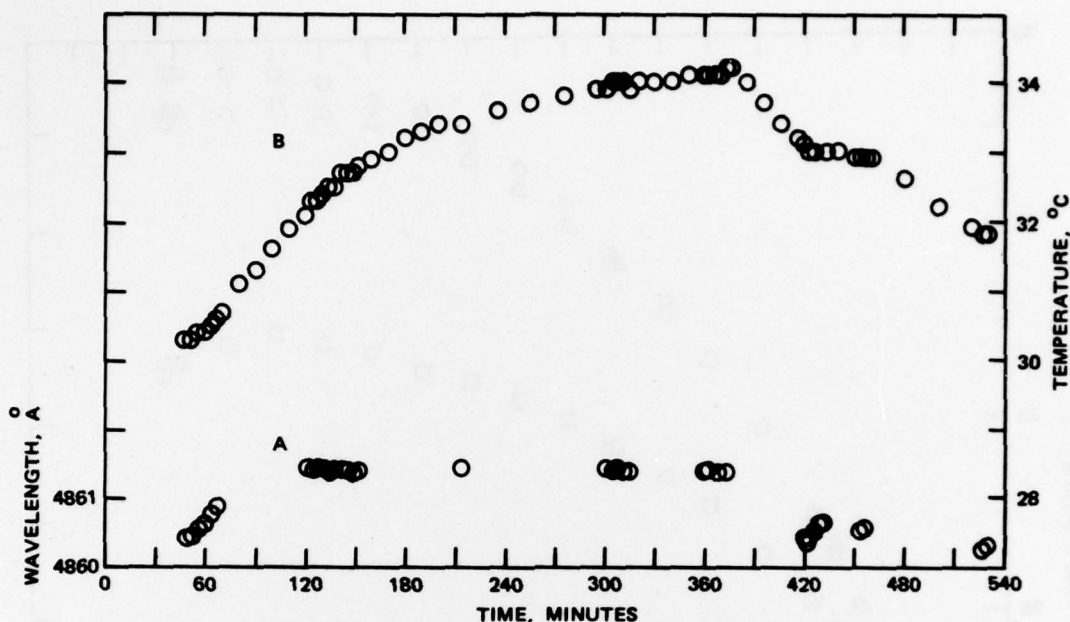


FIGURE 5. Plot of Data Tabulated in Table 3. A. Position of D_{β} line; B. Temperature at front wall of monochromator housing.

off the wavelength stabilized (see the period of 200-400 minutes, Figure 5). Once the scanning was stopped the temperature began to fall and the wavelength λ_c became smaller. Also the shift of λ_c to larger values for scans made in rapid succession resumed. The mean and standard deviation of the line position for scans numbered 35B through 55B are 4861.41 Å and 0.04 Å.

Since the temperature attained by a sample and the time to reach this temperature are of interest in the case of samples whose transmittance and/or spectral response are temperature dependent, the temperature of the sample compartment of the instrument is of interest. The various temperatures monitored are plotted in Figure 6. The data were taken at the same time as the optical measurements shown in Figure 3.

CONCLUSIONS

If excellent stability of the wavelength scale of the instrument is important, then the spectrophotometer must be used in a specified manner. A regime in which the instrument is kept scanning in wavelength at all times leads to stability of wavelength measurements. Another regime leads to nearly constant (very slowly decreasing) values of λ_c .

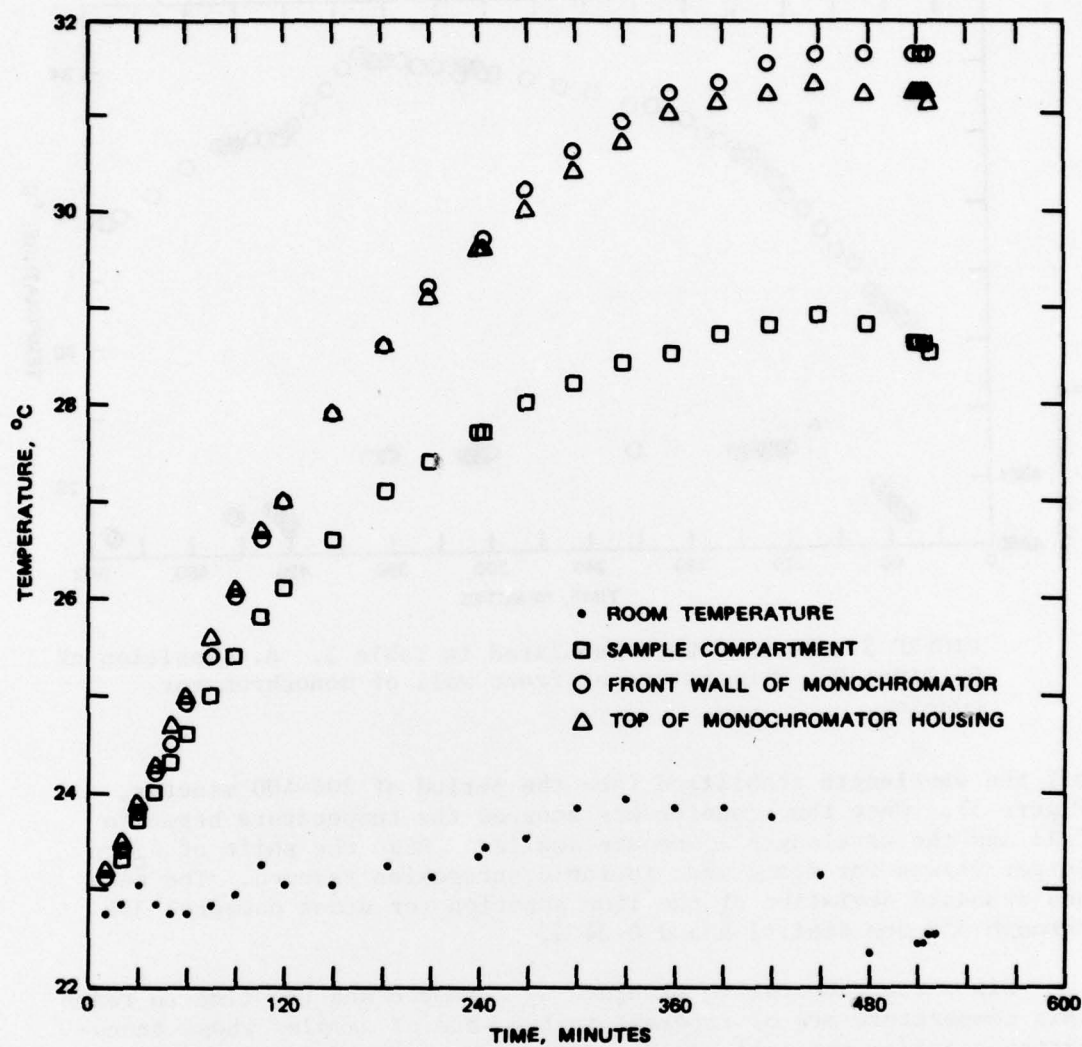


FIGURE 6. Temperature at Various Positions on Spectrophotometer During the Taking of Data Tabulated in Table 1.

during the time the temperature of the instrument is still increasing; this regime is a pattern of short scans (2-3 minutes duration) separated by non-scanning intervals of 30 minutes (Figure 3). It should be noted that the actual value of λ_c differs for the two regimes -- $4861.41 \text{ \AA} \pm 0.04 \text{ \AA}$ for continuous scanning vs. $4860.32 \text{ \AA} \pm 0.01 \text{ \AA}$ for individual short scans made at 30 minute intervals. The accepted value for the D_β line is 4859.99 \AA .²

² National Bureau of Standards. "Errors in Spectrophotometry and Calibration Procedures to Avoid Them," in *Standardization in Spectrophotometry and Luminescence Measurements*, National Bureau of Standards Special Publication 466, May 1977, p. 102.

INITIAL DISTRIBUTION

- 1 Director of Navy Laboratories
- 9 Naval Air Systems Command
 - AIR-30212 (2)
 - AIR-330 (1)
 - AIR-360D, P. L. Luppino (1)
 - AIR-4115 (1)
 - AIR-5332K, W. K. Whiting (1)
 - AIR-536 (1)
 - AIR-954 (2)
- 4 Chief of Naval Operations
- 2 Chief of Naval Material
 - MAT-03 (1)
 - MAT-03PB (1)
- 6 Naval Sea Systems Command
 - SEA-03 (1)
 - SEA-033 (1)
 - SEA-0331 (1)
 - SEA-0332 (1)
 - SEA-09G32 (2)
- 8 Chief of Naval Research, Arlington
 - ONR-100 (1)
 - ONR-102 (1)
 - ONR-401 (1)
 - ONR-420 (1)
 - ONR-439 (1)
 - ONR-460 (1)
 - ONR-472 (1)
 - ONR-473 (1)
- 1 Naval Ocean Systems Center, San Diego (Technical Library)
- 1 Naval Ordnance Station, Indian Head (Technical Library)
- 1 Naval Postgraduate School, Monterey (Technical Library)
- 4 Naval Research Laboratory
 - Technical Library (1)
 - R. A. Patten (1)
 - F. A. Daspit (1)
 - Code 6130 (1)
- 1 Naval Surface Weapons Center, White Oak (Technical Library)
- 1 Naval Weapons Support Center, Crane (Research and Development Department)
- 1 Office of Naval Research Branch Office, Boston
- 1 Office of Naval Research Branch Office, Chicago
- 1 Office of Naval Research Branch Office, Pasadena
- 5 Pacific Missile Test Center, Point Mugu
 - A. R. Burge (1)
 - D. Papcke (1)
 - A. Pignataro (1)
 - J. L. Wadsworth (1)
 - Technical Library (1)

- 1 Army Armament Research and Development Command, Dover (C. E. Newsom)
- 1 Army Missile Research and Development Command, Redstone Arsenal
(Redstone Scientific Information Center, Chief Document Section)
- 1 Army Mobility Equipment Research and Development Center, Fort Belvoir
- 1 White Sands Missile Range (Atmospheric Sciences Laboratory)
- 1 Air Force Flight Test Center, Edwards Air Force Base
- 1 Wright-Patterson Air Force Base (Technical Library)
- 1 Deputy Director of Defense Research and Engineering (T. Walsh)
- 1 Defense Advanced Research Projects Agency, Arlington
- 12 Defense Documentation Center
- 3 National Aeronautics and Space Administration, Wallops Flight Center,
Wallops Island
 - George Foster (1)
 - Charles Manion (1)
 - Thomas Perry (1)
- 8 Goddard Space Flight Center, Greenbelt
 - Code 900, W. Bandeen (1)
 - Code 901, E. Neal (1)
 - Code 912
 - Donald F. Heath (1)
 - E. Hilsenrath (1)
 - Arlin J. Krueger (3)
 - David Wright (1)
- 1 Lewis Research Center (Technical Library)
- 1 National Oceanic and Atmospheric Administration, Boulder (Environmental
Research Laboratory, W. D. Komhyr)
- 1 Barnes Engineering Company, Stamford, CT (E. Wormser)
- 1 Barr Associates, Inc., Concord, MA
- 1 Battelle Memorial Institute, Columbus, OH
- 1 Chemical Propulsion Information Agency, Applied Physics Laboratory,
Silver Spring, MD
- 1 Corion, Holliston, MA
- 1 Environmental Research Institute of Michigan, Ann Arbor, MI
- 2 Honeywell, Defense Electronics Division, Lexington, MA
 - Sol Norman (1)
 - David Reilly (1)
- 1 IIT Research Institute, Chicago, IL (Technical Library)
- 1 Institute for Defense Analyses, Arlington, VA (L. M. Biberman)
- 1 Jet Propulsion Laboratory, CIT, Pasadena, CA (Technical Library)
- 1 Los Alamos Scientific Laboratory, Los Alamos, NM (Technical Library)
- 1 Lunar and Planetary Laboratory, University of Arizona, Tucson, AZ
(L. Dunkelman)
- 1 New Mexico State University, Las Cruces, NM (Physical Sciences
Laboratory, B. G. Gammill)
- 2 Optical Coating Laboratory, Inc., Santa Rosa, CA
 - B. E. Michel (1)
 - Alfred Thelen (1)
- 1 SRI International, Menlo Park, CA (Technical Library)

2 SWL, Division of General Research Corporation, McLean, VA

O. T. Inge (1)

R. A. Rollin, Jr. (1)

1 Santa Barbara Research Center, Goleta, CA

1 SenTran Company, Santa Barbara, CA (Peter G. Simeth)

1 The Aerospace Corporation, Los Angeles, CA (Technical Library)

3 Varian, Instrument Division, Downey, CA

A. Koenig (1)

Joseph Laurinovics (1)

D. Sparks (1)